

Into the Wilds of Alpha Spectroscopy

Surprising treasures in the details


David K. Baltz
Chief Technologist
Bladewerx LLC
Rio Rancho, NM



More than an annoyance

Alpha-emitting radon decay products can be a nuisance when monitoring for transuranics, but there are some surprising benefits to the most common of background interferences. We will cover a few of them here and delve into the details of some of the most promising.


Radon/Thoron Background Spectrum

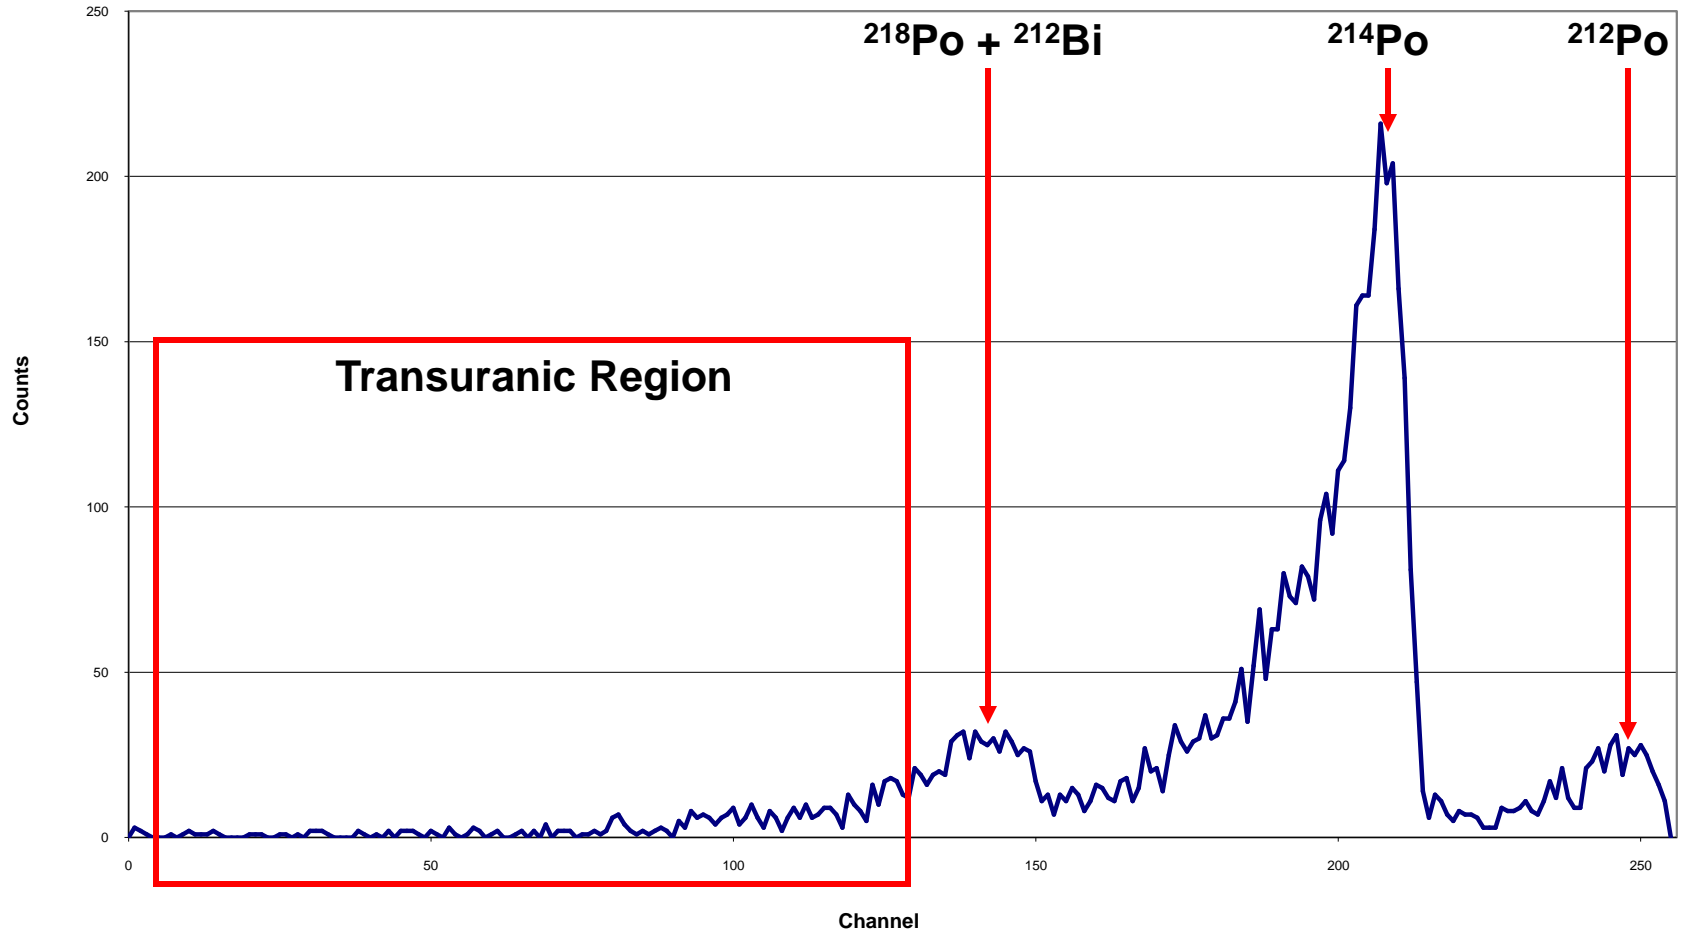

Benefits of RDP Background?

Admittedly, we will never be able to eliminate RDP background, but when we are looking for a few DPM from transuranics against a background of 200 to 2000 DPM of RDP, what benefits could there possibly be?

Benefit #1: A calibration reference

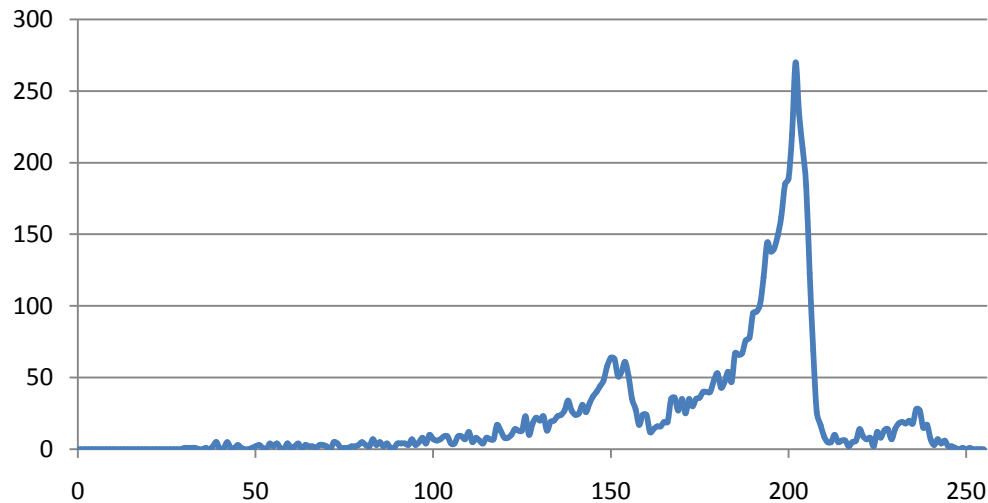


- Radon progeny provide two/three energy reference points.
- If the peaks move, so will the isotope-of-interest.

What can be done with this?

- Energy calibration without sources
- Automatic energy offset adjustments for temperature/pressure
- Automatic compensation for changes in altitude


Benefit #2: Energy Compensation

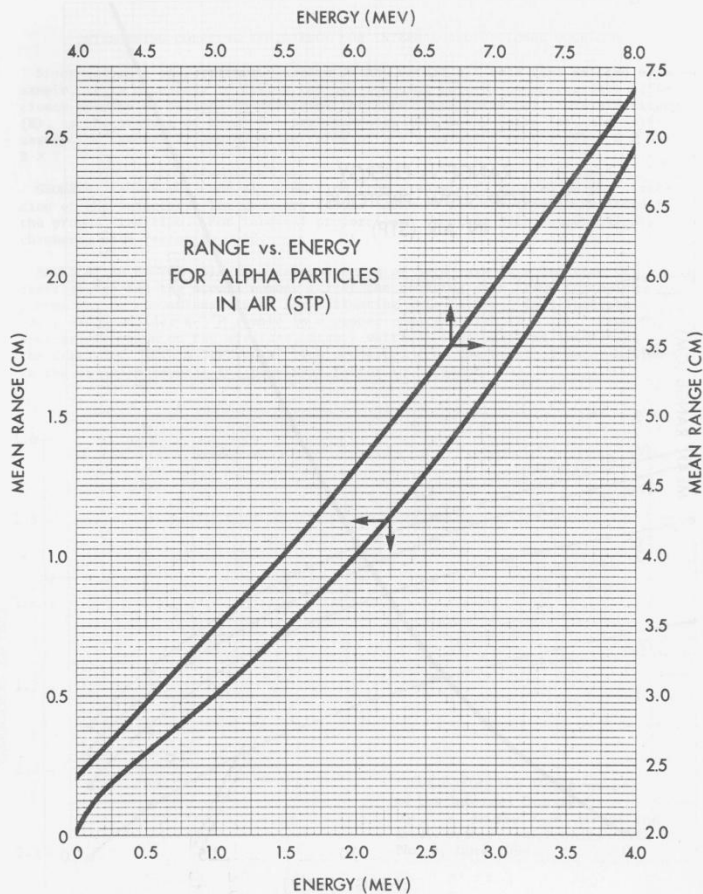

Source: Radiological Health Handbook

125

- Apart from electronic nonlinearity, alpha particle energy loss in air is nonlinear.
- Less energetic alphas have more attenuation per millimeter than more energetic alphas.
- The shape of the ^{218}Po tail gives us information about this attenuation so we can better predict where the peak of a specific radionuclide will fall.

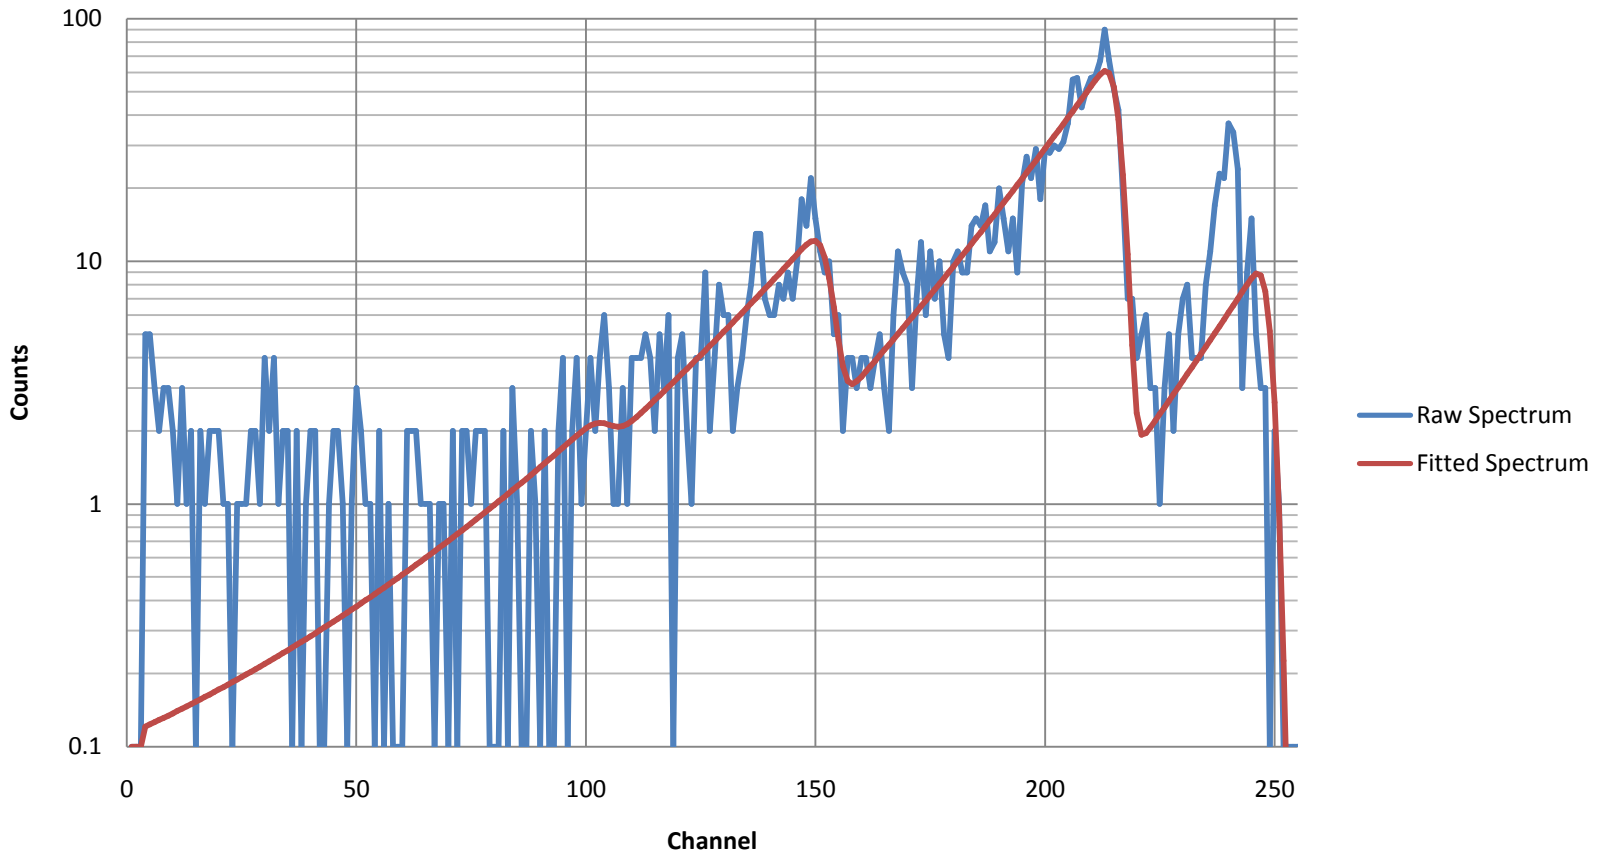

- Adjustment of ^{218}Po tail yields an energy non-linearity correction factor which reduces bias in isotope-of-interest fit.

Benefit #3: Beta compensation

Accurate compensation of a gross beta channel for beta-emitting RDPs (^{214}Pb , ^{214}Bi , ^{212}Bi , ^{208}Tl)

- ^{214}Pb counts can be estimated by ^{218}Po and ^{214}Po concentrations and equilibrium level
- $^{214}\text{Bi} = ^{214}\text{Po}$
- $^{212}\text{Bi} = ^{212}\text{Po} \times 1/0.64 \times 0.35$
- $^{208}\text{Tl} = ^{212}\text{Po} \times 0.36/0.64$ (with 3.05 min $T_{1/2}$)

Benefit #4: Equilibrium information


- The ratios of the ^{218}Po , ^{214}Po , and ^{212}Po peaks can give us an indication of the concentration equilibrium.
- Full equilibrium yields a $^{214}\text{Po}/^{218}\text{Po}$ ratio of 6.47 (must be adjusted for ^{212}Bi)
- Lesser ratios indicate partial equilibrium
- In HEPA-filtered air, equilibrium level can be accurately estimated.

Benefit #5: Particulate size information

- When the concentration equilibrium is known and a filter media with significant sub-micron penetration is used, the $^{218}\text{Po}/^{214}\text{Po}$ ratio can provide sizing clues about the particulates to which the RDP are attaching.
- Comparison with 'full collection' filter media can add to the picture.


Polonium Ratio

Closed room w/no work activity

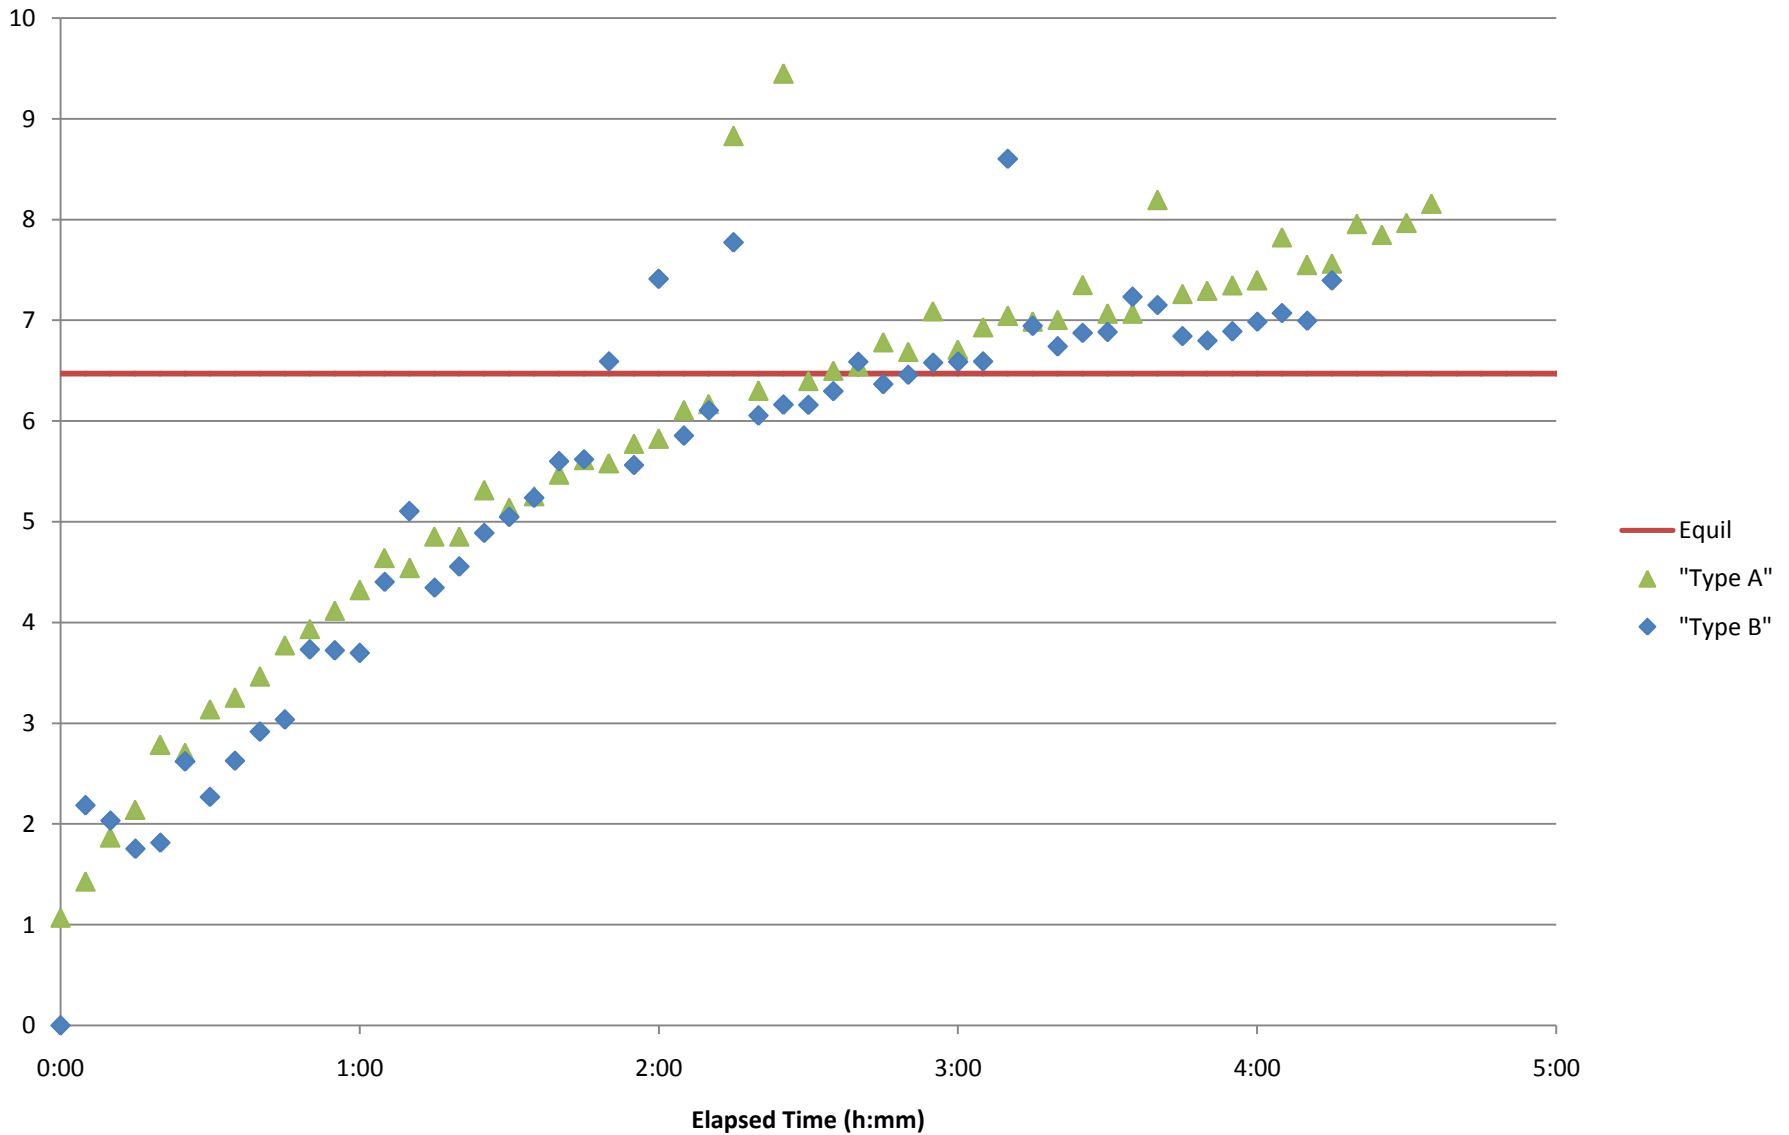


Spectrum Comparison

Closed room w/no work activity

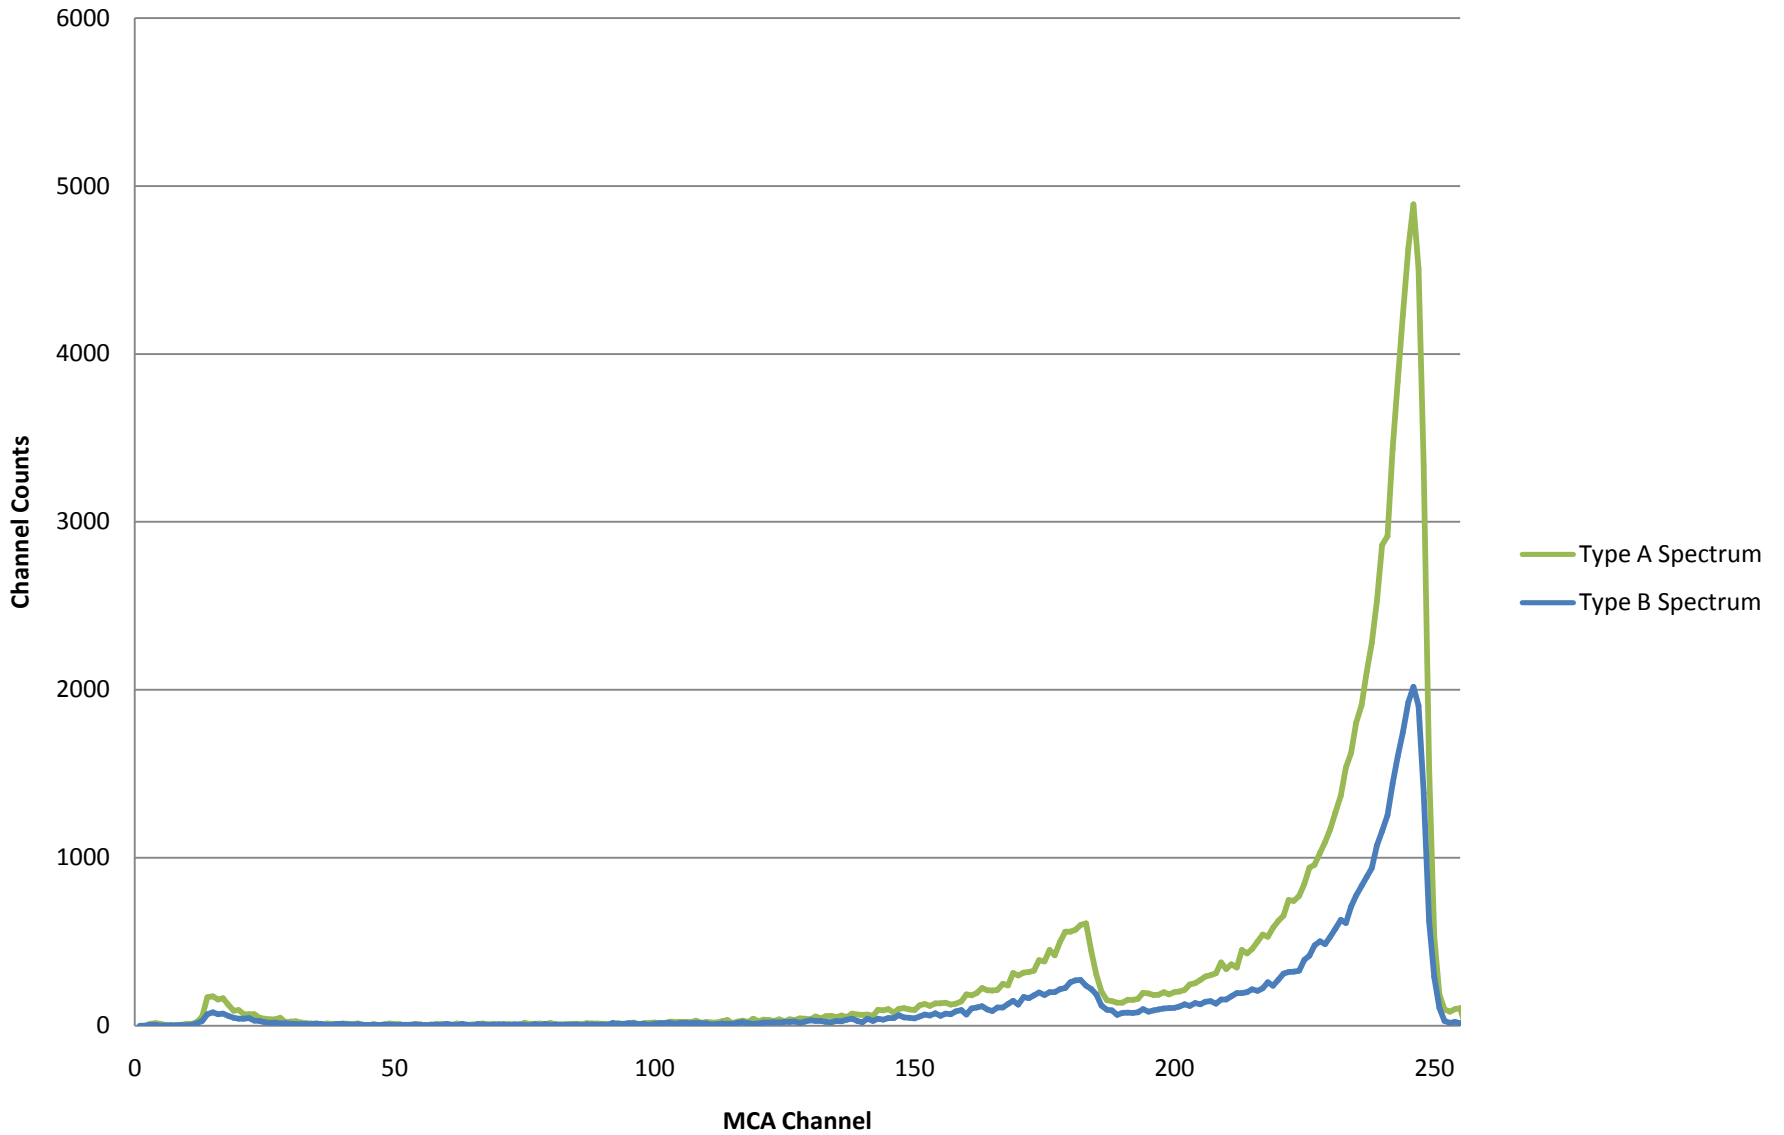


Polonium Ratio

Open room w/ work activity

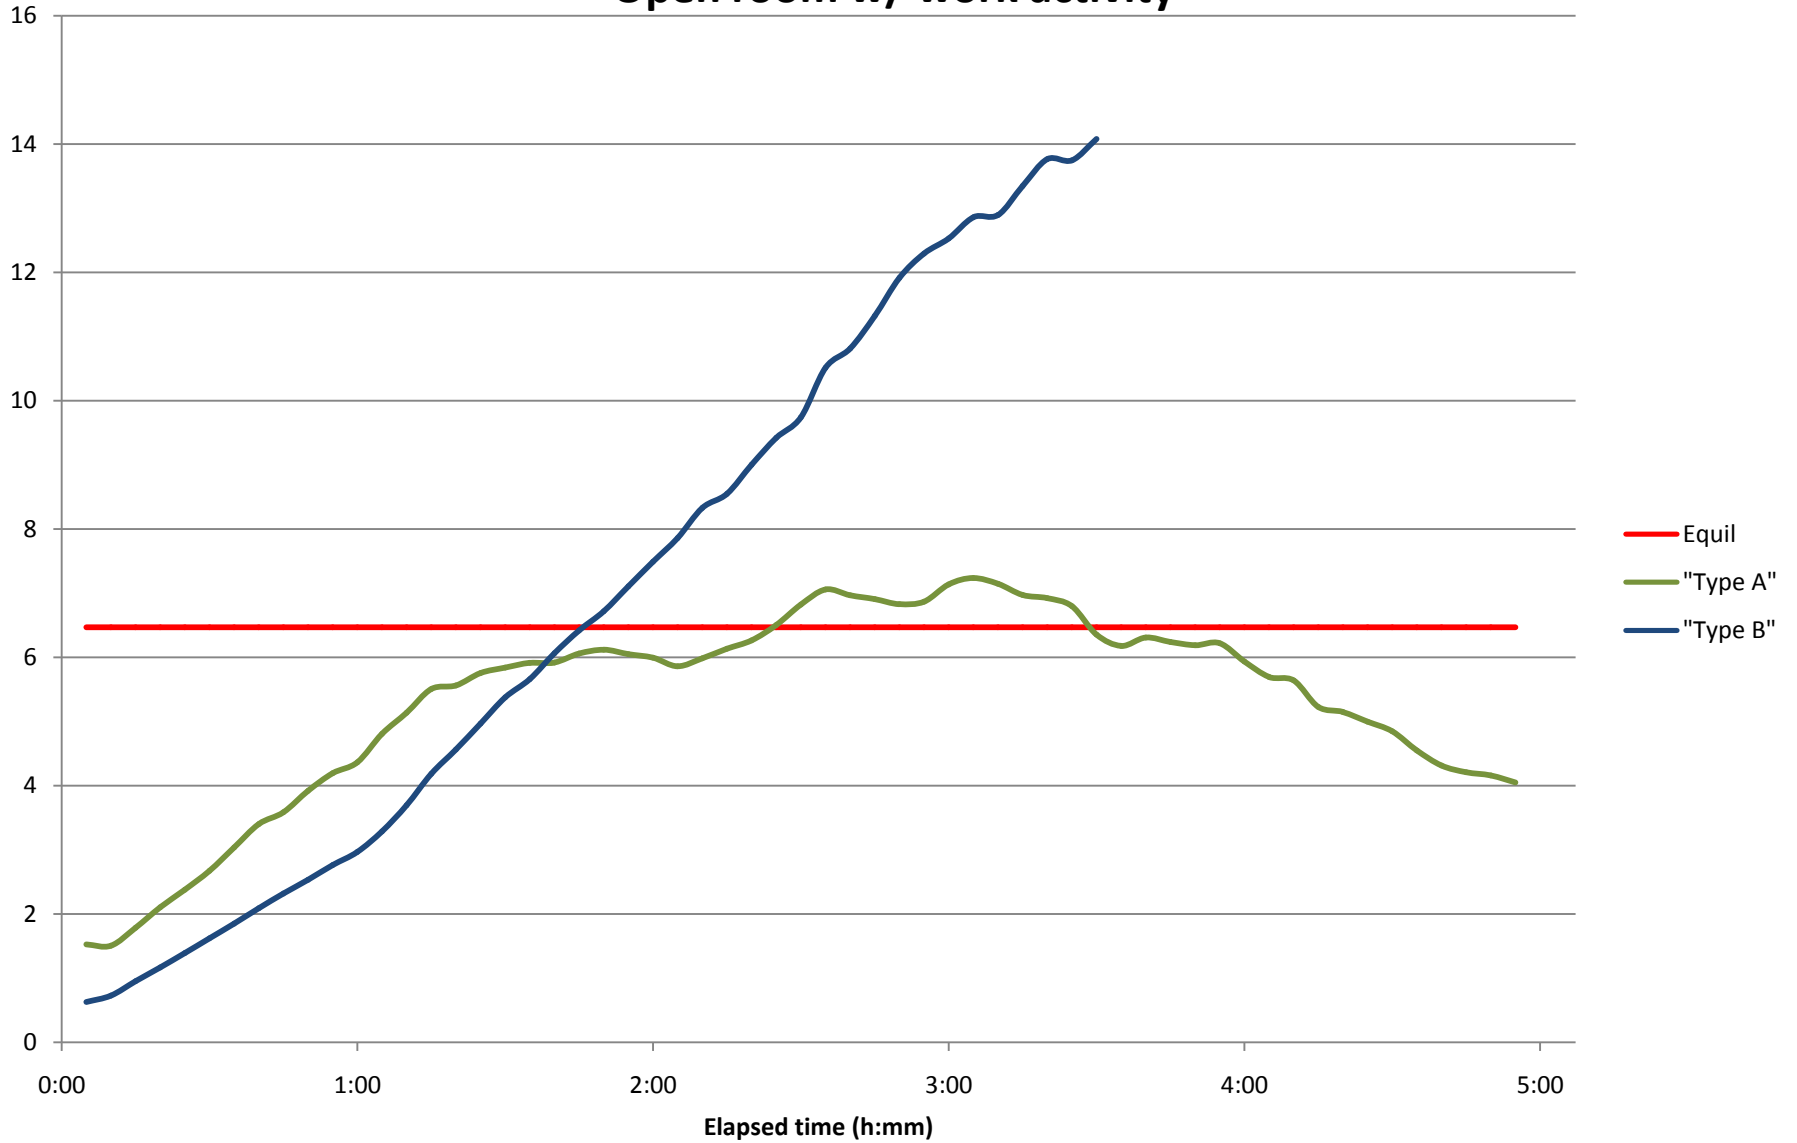

Spectrum Comparison

Open room w/ work activity

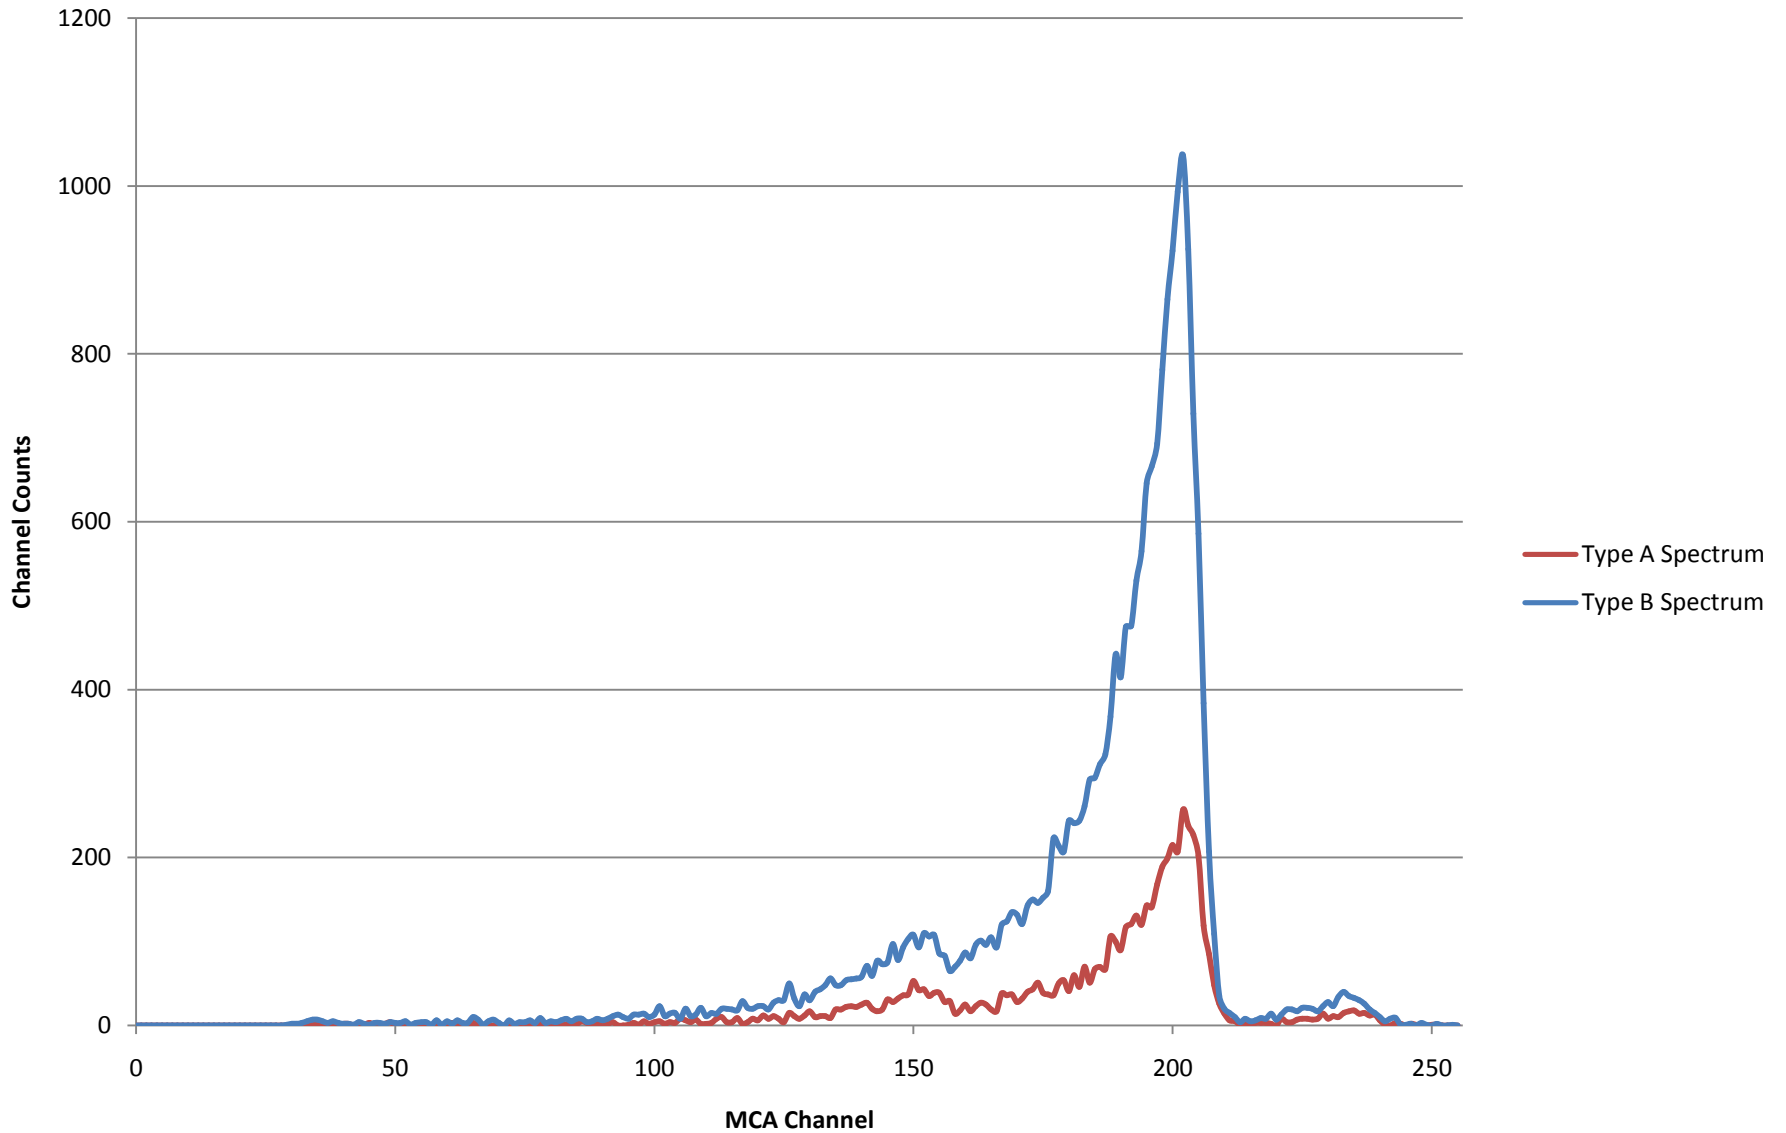

Discussion

- Is source-less energy calibration useful?
- For Radon background subtraction of a beta channel to be truly practical, a two point beta efficiency should be done. Is it worth the effort?
- What is more useful to the HP, knowing the equilibrium, or knowing the particulate sizing?